LEVEL 5 - LOCK LEVEL :

Display	Name & Description	Range	Display condition	Default value
[redacted]	User ID	0000 to 9999	——	0000
[redacted]	Lock Level 0	UNLK/READ/LOCK	——	UNLK
[redacted]	Lock Level 1	UNLK/READ/LOCK	——	UNLK
[redacted]	Lock Level 2	UNLK/READ/LOCK	——	UNLK
[redacted]	Lock Level 3	UNLK/READ/LOCK	——	UNLK
[redacted]	Lock Level 4	UNLK/READ/LOCK	——	UNLK

NOTE :
UNLK - Full access to the particular level / parameter.
READ - Particular level / parameter can be read but not edited.
LOCK - No access to the particular level / parameter.

IDM Level

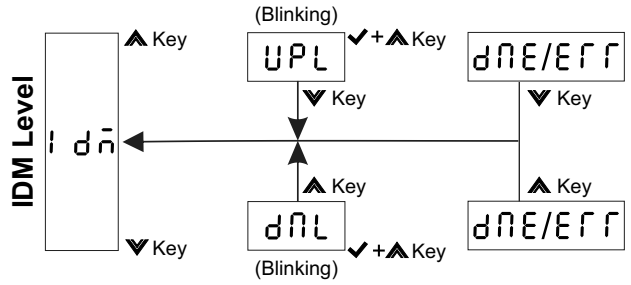

Display	Parameter Description
Idn	Independent Downloader Module
UPL	Upload from product to IDM
dNL	Download from IDM to product
dNE	Operation Successful
ERR	Operation Unsuccessful

Note :
1) IDM Level - IDM should be connected before powering on the unit to enter in IDM level
2) Long press ⮝ or ⮟ key for 3 sec to exit from IDM mode.

Caution : After Downloading, switch of the unit and then remove the IDM

CALIBRATION CERTIFICATE

selec

Model No : PIC352-11-U-X-1

Claimed Accuracy : ± 0.1 % of full scale ±1 digit (After 20min warmup time)

Standard used for calibration of the product is traceable to NABL

The calibration of this unit has been verified at the following values:

SENSOR	CALIBRATION TEMP (°C) (0.1 resolution)	DISPLAY VALUE (°C)	SENSOR	CALIBRATION VALUE (0.1 resolution)	DISPLAY VALUE
K	35.0	35.0	Voltage (VDC)	0.0	0.0
	700.0	700.0		10.0	10.0
	1350	1350			
PT100 / PT1000	0.0	0.0	Current (mA)	0.0	0.0
	500.0	500.0		20.0	20.0
	800.0	800.0			

The thermocouple / RTD curves are linearised in this microprocessor based product, and hence the values interpolated between the readings shown above are also equally accurate, at every point in the curve.

Unit is accepted as accuracy is withing the specified limit of claimed accuracy and certificate is valid upto one year from the date of issue.